

TB4 Series 2

User Manual

Table of Contents

I	Disclaimer	3
II	Scope of Delivery	4
III	Safety Instructions	5
Part I	Introduction	6
Part II	Installation	7
2.1	Unpacking your TB4 Rain Gauge	7
2.2	Site Selection and Setup	7
Part III	Configuration	11
3.1	Calibration	11
3.2	Field Calibration Device	11
Part IV	Operation	12
4.1	Test Operation	12
4.2	Electrical	12
Part V	Maintenance	13
Part VI	Repair	15
6.1	TB4 Part List	15
Part VII	Technical Data	22
Part VIII	Obligations of the Operator and Disposal	23
8.1	Obligations of the Operator	23
8.2	Dismantling / Disposal	23

I Disclaimer

The information provided in this manual was deemed accurate as of the publication date. However, updates to this information may have occurred.

This manual does not include all of the details of design, production, or variation of the equipment nor does it cover every possible situation which may arise during installation, operation or maintenance. HyQuest Solutions shall not be liable for any incidental, indirect, special or consequential damages whatsoever arising out of or related to this documentation and the information contained in it, even if HyQuest Solutions has been advised of the possibility of such damages.

Any errors found in any HyQuest Solutions product should be reported to HyQuest Solutions where every effort will be made to quickly resolve the problem.

Copyright Notice: No parts of this work may be reproduced in any form or by any means without the written permission of the publisher. HyQuest Solutions waives copyright for users to print out parts of the documentation in hard copy for their own use only.

Trademark Notice: HyQuest Solutions (HS) and KISTERS products and services referred to in this document are trademarks or registered trademarks of HyQuest Solutions or KISTERS AG. Other product names used may or may not be the trademarks of their respective owners.

© 2020 HyQuest Solutions, a KISTERS Group Company. Any rights not expressly granted herein are reserved.


II Scope of Delivery

- TB4/Series II/T Rain gauge
- TB311/5 5 metre connecting lead


III Safety Instructions

- Read the user manual including all operating instructions prior to installing, connecting and powering up the HyQuest Solutions TB4_Series2. The manual provides information on how to operate the product. The manual is intended to be used by qualified personnel, i.e. personnel that have been adequately trained, are sufficiently familiar with installation, mounting, wiring, powering up and operation of the product.
- Keep the user manual on hand for later reference!
- If you encounter problems understanding the information in the manual (or part thereof), please consult the manufacturer or its appointed reseller for further support.
- HyQuest Solutions TB4_Series2 is intended to be used in hydrometeorological or environmental monitoring applications.
- Before starting to work, you have to check the functioning and integrity of the system.
 - Check for visible defects on the TB4_Series2, this may or may not include any or all of the following mounting facilities, connectors and connections, mechanical parts, internal or external communication devices, power supplies or power supply lines, etc.
 - If defects are found that jeopardize the operational safety, work must be stopped. This is true for defects found before starting to work as well as for defects found while working.
- Do not use the HyQuest Solutions TB4_Series2 in areas where there is a danger of explosion.
- The present user manual specifies environmental/climatic operating conditions as well as mechanical and electrical conditions. Installation, wiring, powering up and operating the HyQuest Solutions TB4_Series2 must strictly comply with these specifications.
- Perform maintenance only when tools or machinery are not in operation.
- If guards are removed to perform maintenance, replace them immediately after servicing.
- Never make any electrical or mechanical diagnostics, inspections or repairs under any circumstances. Return the sensor to the manufacturer's named repair centre. You can find information on how to return items for repair in the relevant section of the HyQuest Solutions web site.



-  Disposal instructions: After taking the HyQuest Solutions TB4_Series2 out of service, it must be disposed of in compliance with local waste and environmental regulations. The HyQuest Solutions TB4_Series2 is never to be disposed in household waste!



-  Inputs and outputs of the device are protected against electric discharges and surges (so-called ESD). Do not touch any part of the electronic components! If you need to touch any part, please discharge yourself, i.e. by touching grounded metal parts.

1 Introduction

Thank you for choosing our product. We hope you will enjoy using the device.



HyQuest Solutions manufactures, sells, installs and operates quality instrumentation, data loggers and communication technology. Products are designed with passion for environmental monitoring and with a deep understanding of the quality, accuracy and robustness needed to fulfil the requirements of measurement practitioners in the field.

The present User Manual will help you understand, install and deploy the device. If, however, you feel that a particular information is missing, incomplete or confusing, please do not hesitate to contact us for further support!

HyQuest Solutions' TB4 Series II is a high-quality tipping bucket rain gauge for measuring rainfall in urban and rural locations. Due to the integrated syphon, the gauge delivers high levels of accuracy across a broad range of rainfall intensities.

2 Installation

This chapter contains the following subsections:

- [Unpacking your TB4 Rain Gauge](#) 
- [Site Selection and Setup](#) 

2.1 Unpacking your TB4 Rain Gauge

This package should contain:

- TB4/Series II/T Rain gauge
- TB311/5 5 metre connecting lead

Please verify you have received these items and that the Tipping Bucket Rain gauge resolution is as ordered.

To prepare the Tipping Bucket Rain gauge for installation:

- lift the unit from the carton and place on secure surface
- remove polythene bag
- loosen the three enclosure securing screws and back them off until screw head is clear of the enclosure.
- lift the enclosure from the gauge
- carefully remove the elastic band/support pad from the bucket.

Your Tipping Bucket Rain gauge is now ready for installation.

2.2 Site Selection and Setup

Site Selection

Rainfall measurements are intended to be representative of the actual rain falling on a given area. Some of the more important factors which influence the representativeness of a gauge are as follows:

- Site the gauge on level ground where possible. Avoid sloping sites.
- Site should have adequate protection from strong winds.
- Site should be free of large obstructions such as buildings and trees.
- Provide suitable ground surface to avoid splashing into the gauge.

Setting up

- Install the gauge on the foundation. A suggested foundation is shown in Diagram 1.
- Loosen the three enclosure securing screws and the enclosure.
- The gauge is provided with a bull's eye level. Adjust the nuts on mounting bolts until gauge is level.
- Connect lead to the Rain Gauge terminals, refer to Diagram 7, and to the recording device, in accordance with manufacturer's instructions.

Floor Mount:

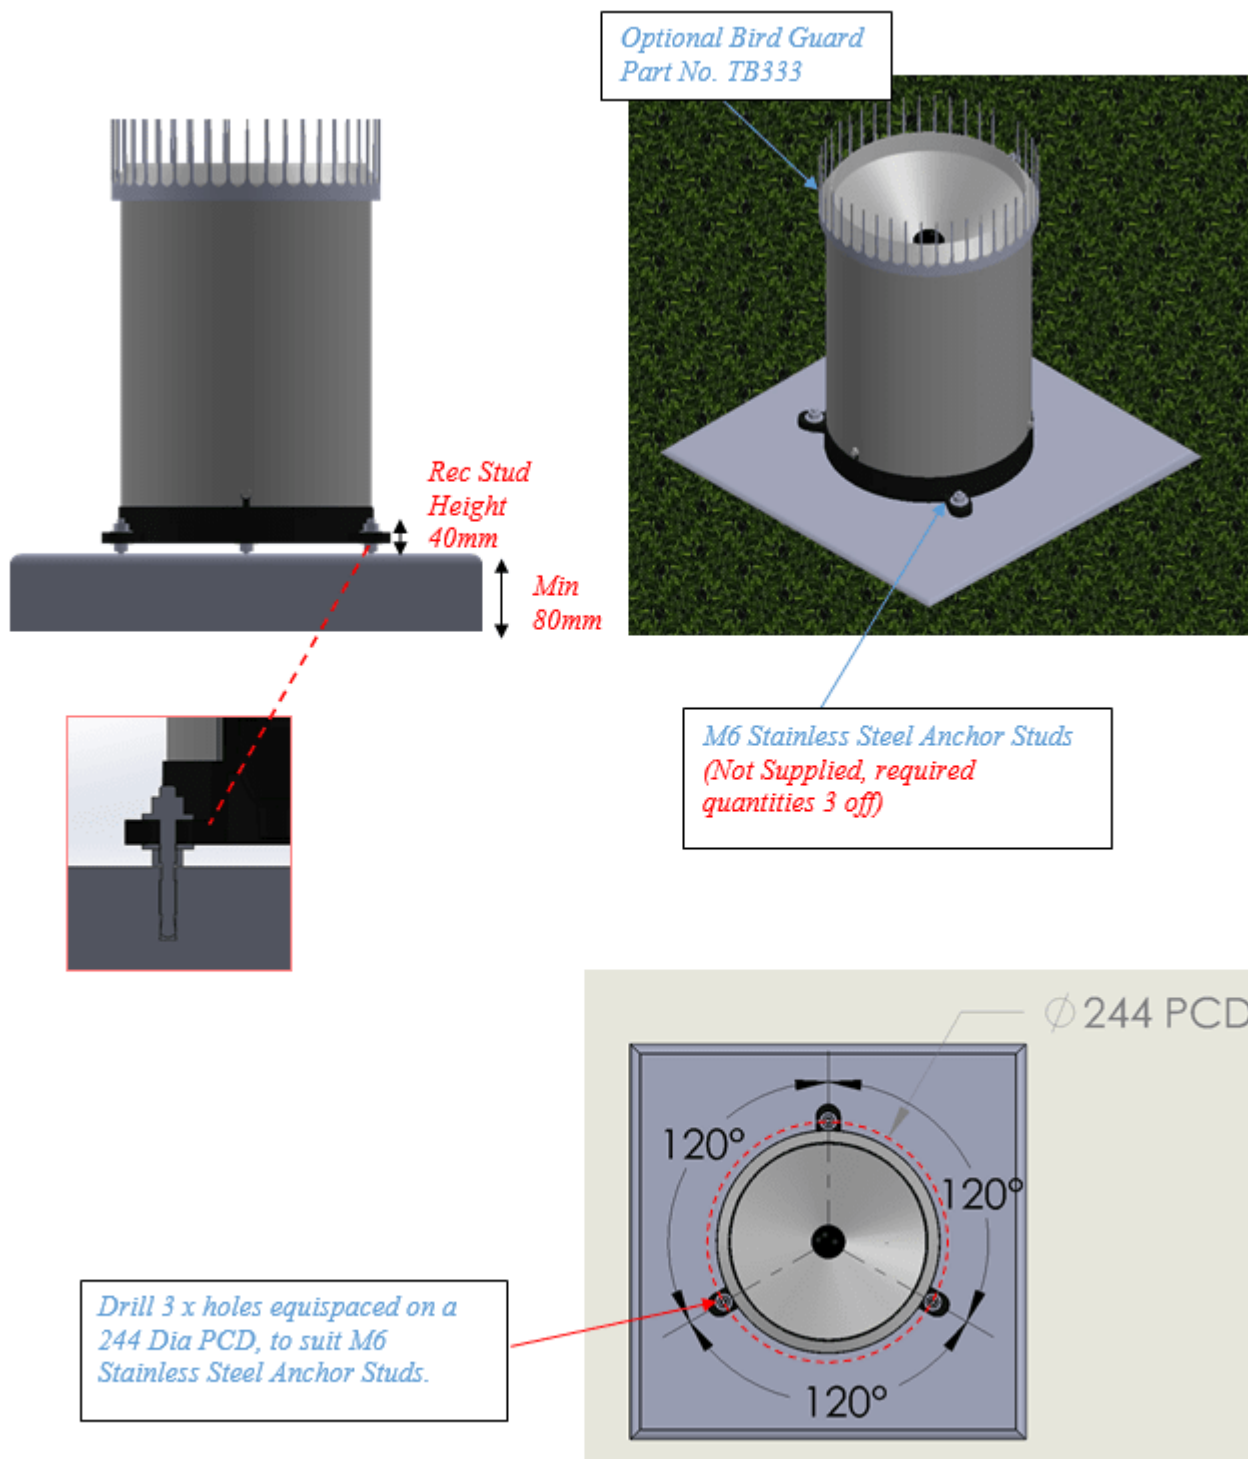


Diagram 1

Pole Mount:

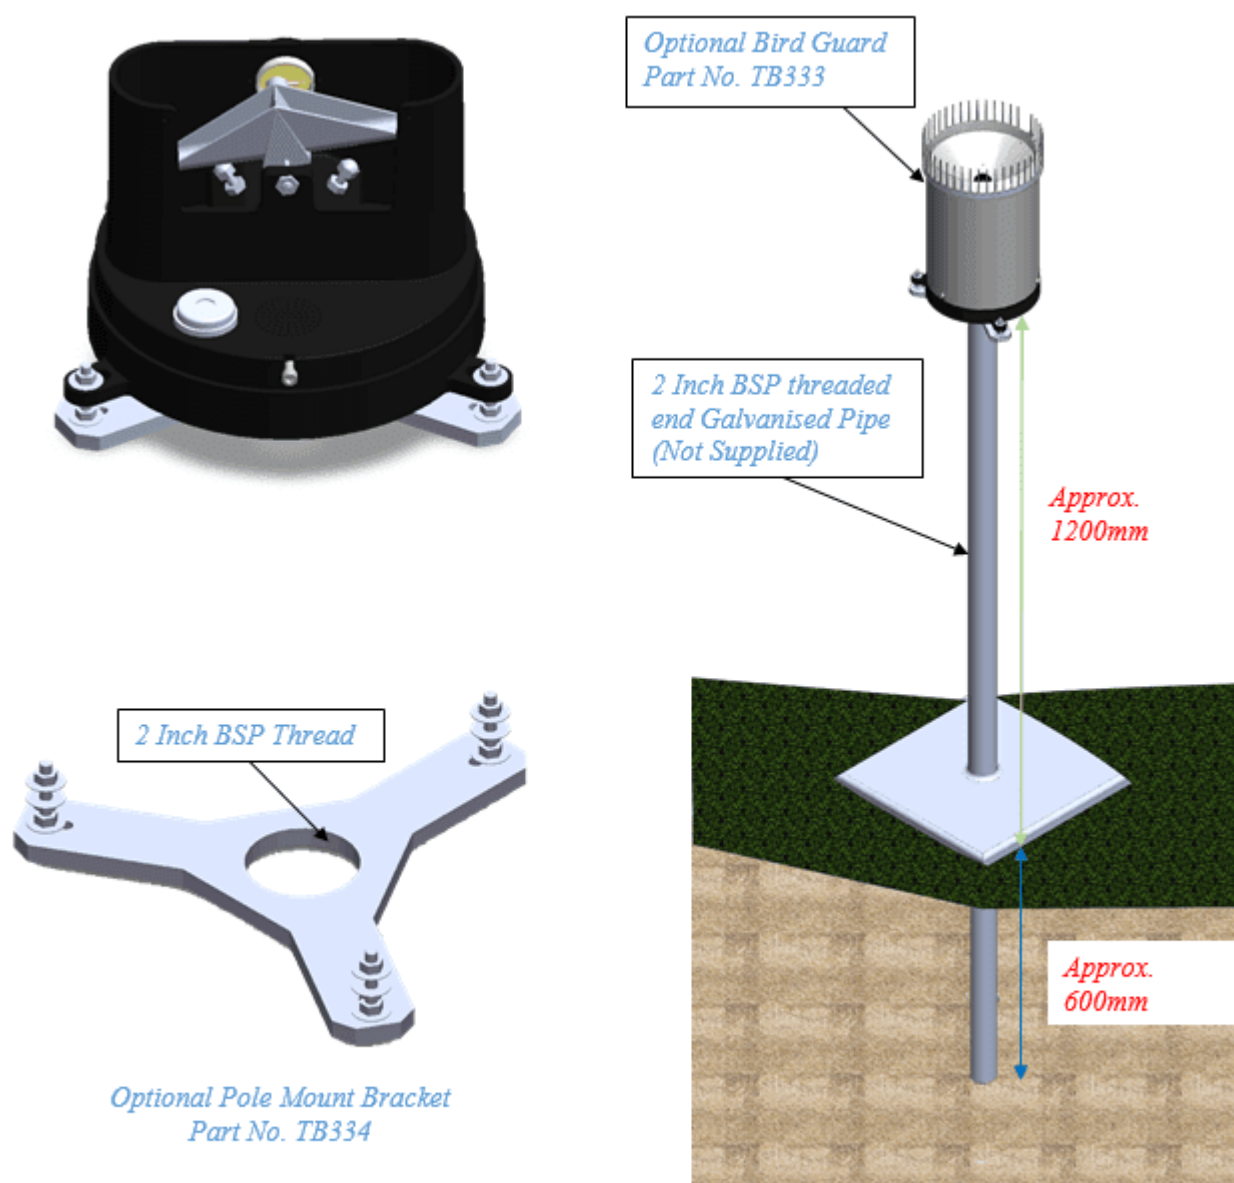
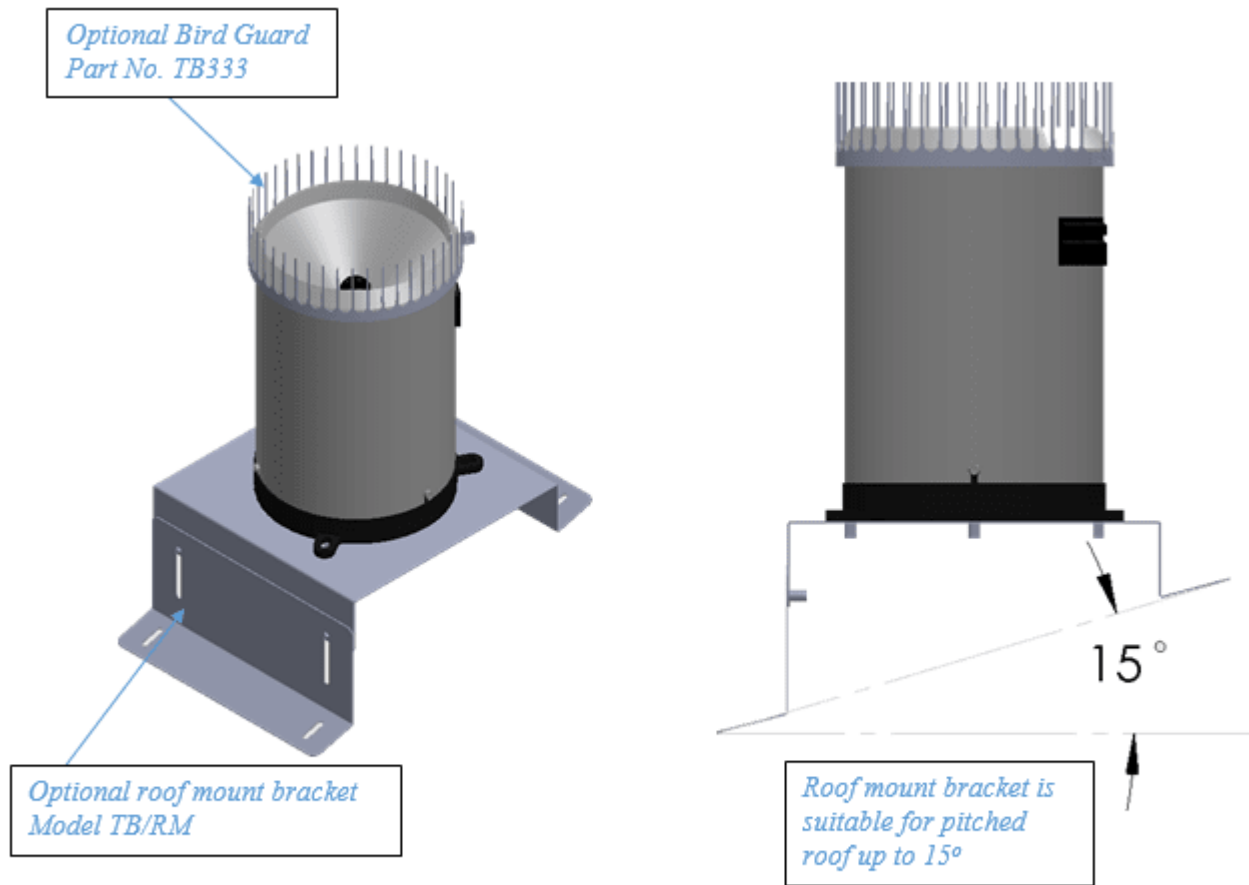


Diagram 2

Roof Mount:

The Rain Gauge can also be mounted on a pitched roof with maximum angle of 15 degrees.

*Diagram 3*

3 Configuration

This chapter contains the following subsections:

- [Calibration](#)
- [Field Calibration Device](#)

3.1 Calibration

All gauges have been calibrated by HyQuest Solutions Pty Ltd, prior to despatch.


The following products and services are available from HyQuest Solutions Pty Ltd:

- Field Calibration Device, Model FCD, for routine field check calibrations, supplied with operating instruction sheet refers to [FIELD CALIBRATION DEVICE](#)
- Laboratory Calibration Unit, Model TB340A, for calibration after servicing in workshops, supplied with operating manual.
- Recalibration Service at HyQuest Solutions' factory.

Please contact either HyQuest Solutions Pty Ltd or our local distributor for further information.

3.2 Field Calibration Device

NOTE: PLEASE WET RAIN GAUGE PRIOR TO CALIBRATION

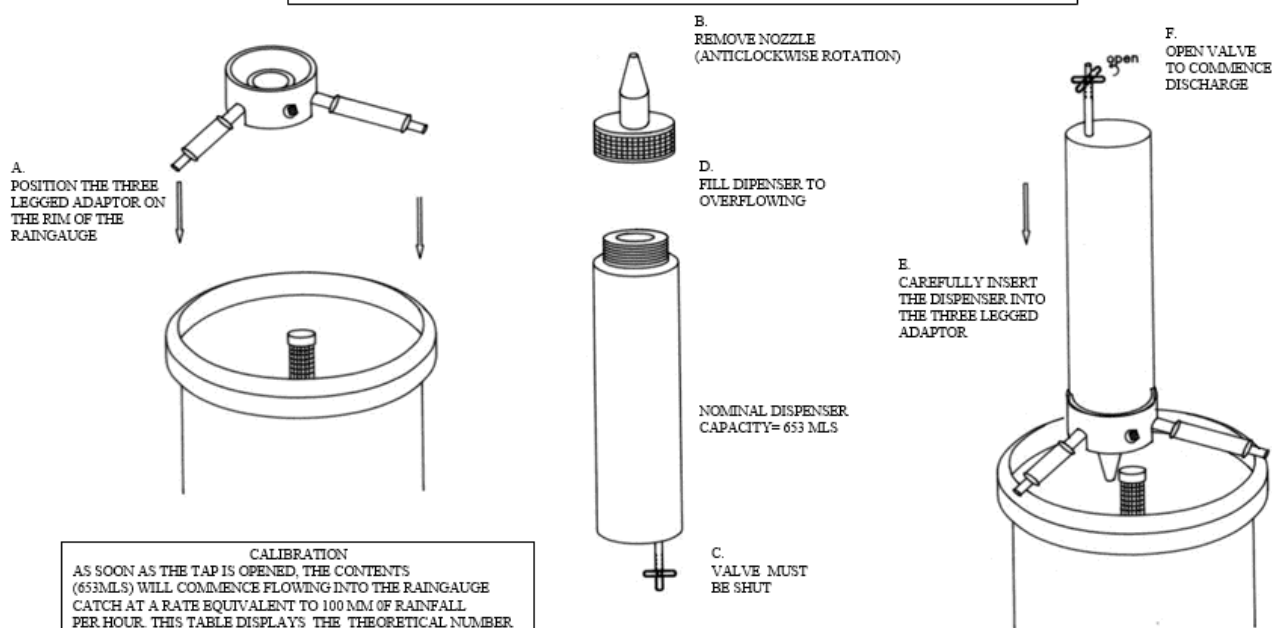

CALIBRATION		
AS SOON AS THE TAP IS OPENED, THE CONTENTS (653MLs) WILL COMMENCE FLOWING INTO THE RAINGAUGE CATCH AT A RATE EQUIVALENT TO 100 MM OF RAINFALL PER HOUR. THIS TABLE DISPLAYS THE THEORETICAL NUMBER OF BUCKET TIPS THAT SHOULD BE ACHIEVED.		
THEORETICAL NUMBER OF TIPS		
BUCKET SIZE	200 MM CATCH	203 MM (8")
0.2 MM	103.9	100.9
0.5 MM	41.6	40.4
0.01 INCH	81.8	79.4
IF THE OBSERVED RESULTS ARE UNACCEPTABLE THEN REFER TO THE RAINGAUGE INSTRUCTION MANUAL FOR APPROPRIATE ADJUSTMENTS		

INSTRUCTION FOR TIPPING BUCKET

RAIN GAUGE FIELD CALIBRATOR (FCD)

4 Operation

This chapter contains the following subsections:

- [Test Operation](#) ¹²
- [Electrical](#) ¹²


4.1 Test Operation

- Manually tip the bucket a number of times, ensuring that each tip is being recorded and that the tilting mechanism is operating freely.
- Replace and secure the enclosure.

4.2 Electrical

Dual reed switches are provided for several reasons:

- Two isolated switches permit the control of two separate circuits; e.g. a local counter and a telemetry circuit.
- Parallel connection of both switches increases the current carrying capacity of the contact system if required.
- Parallel switch operation confers a degree of redundancy in locations where data from the Rain gauge is critical to flood warning etc.

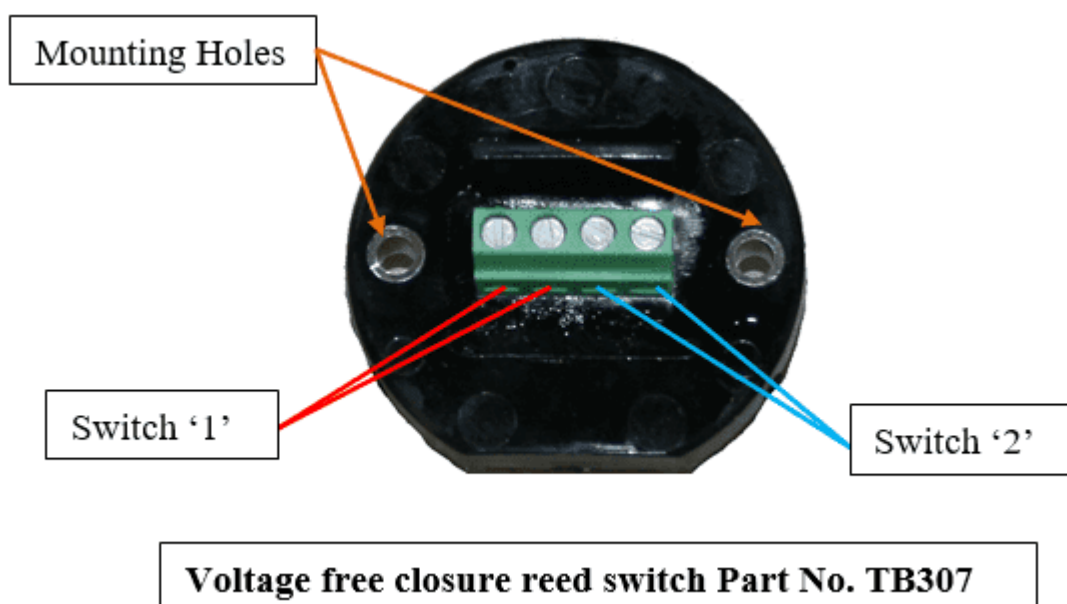

5 Maintenance

The only routine maintenance required is cleaning. The following items should be checked regularly for cleanliness:

- Catch filter
- Syphon (refer diagram 5)
- Interior of bucket
- Top surface of adjusting screws
- Enclosure locking screws - lightly lubricate after cleaning
- All insect screens

Dismantle Details

- a. Unscrew nut
- b. Lightly press stem down on surface until stem pops out of syphon body.
- c. Remove stem from syphon body.
- d. Unscrew cap
- e. Clean all items

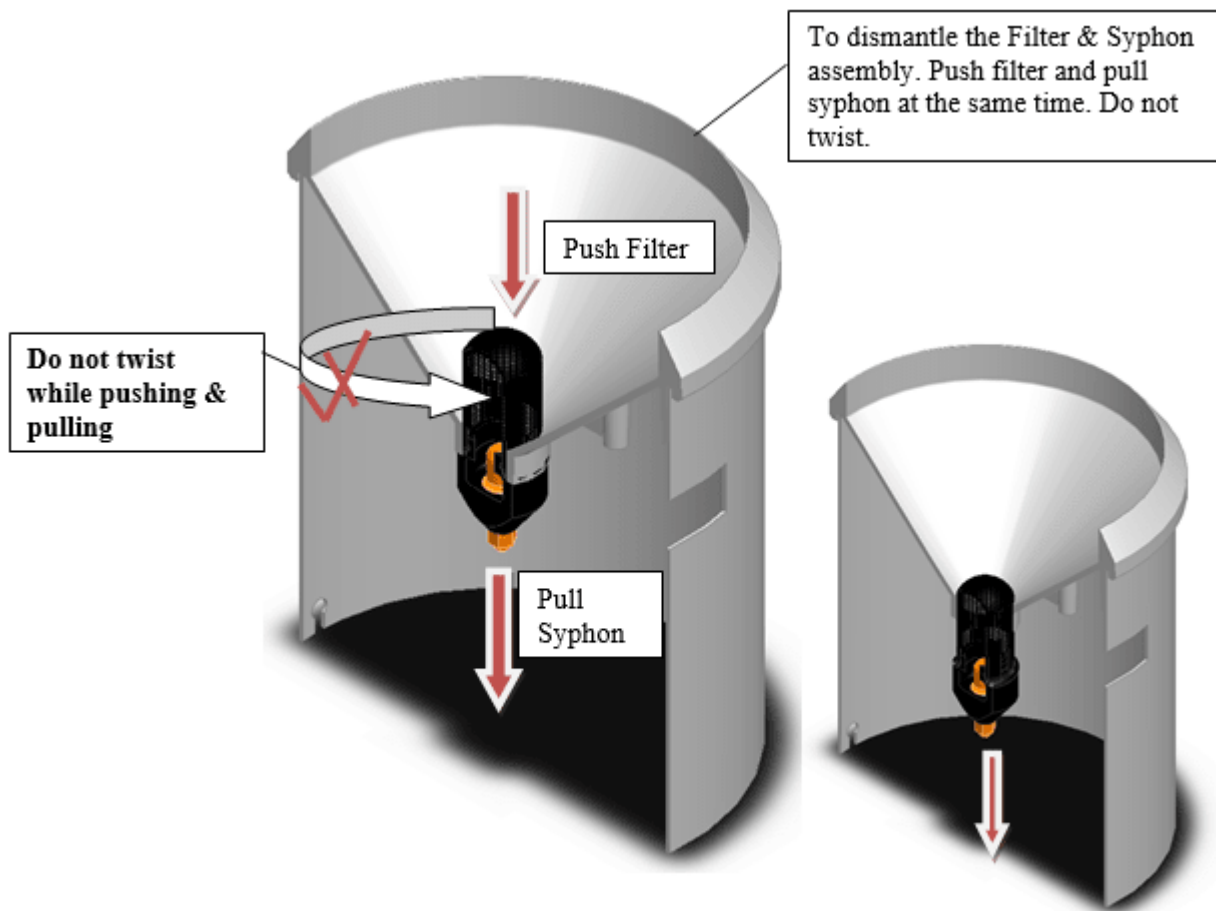


Diagram 4

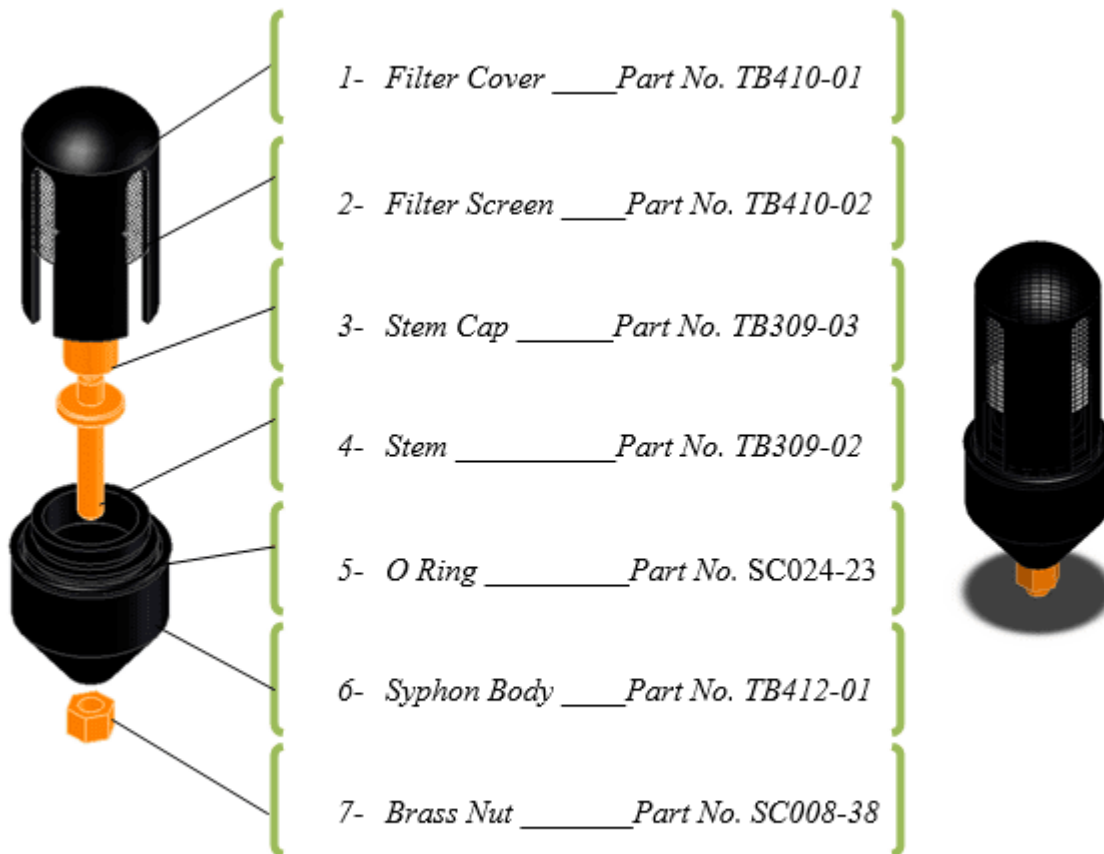


Diagram 5

Assembly Details

- Screw cap on stem. Finger tight only.
- Push stem into syphon body.
- Replace nut and tighten. Do not over tighten.

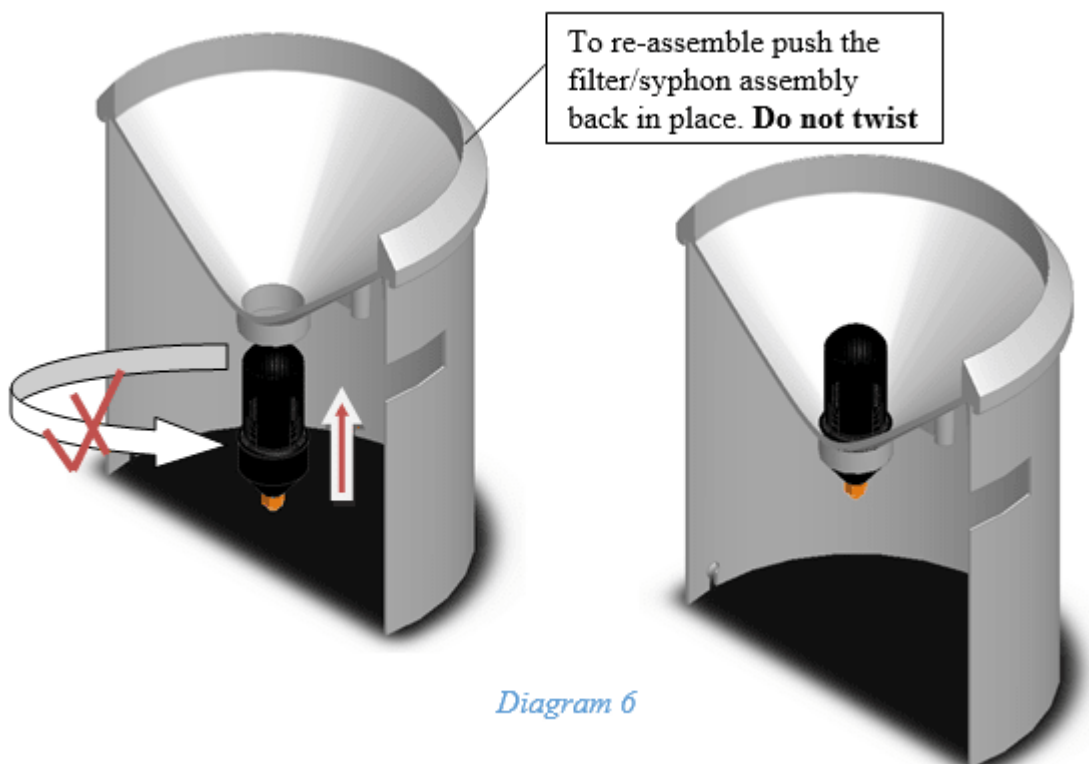


Diagram 6

6 Repair

HyQuest Solutions precision instruments and data loggers are produced in quality-controlled processes. All HyQuest Solutions production and assembly sites in Australia, New Zealand and Europe are ISO 90001 certified. All equipment is factory tested and/or factory calibrated before it is shipped to the client. This ensures that HyQuest Solutions products perform to their fullest capacity when delivered.

Despite HyQuest Solutions most rigorous quality assurance (QA), malfunction may occur within or outside of the warranty period. In rare cases, a product may not be delivered in accordance with your order.

In such cases HyQuest Solutions' return and repair policy applies. For you as a customer, this means the following:

1. Contact HyQuest Solutions using the Repair Request Form made available online:
https://www.hyquestsolutions.eu/fileadmin/Form/Telemetry_Solution_app.jpg.pdf
 In response you will receive a reference number that must be referenced on all further correspondence and on the freight documents accompanying your return shipment.
2. Please provide as much information and/or clear instructions within the return paperwork. This will assist our test engineers with their diagnosis.
3. Please do not ship the goods prior to obtaining the reference number. HyQuest Solutions will not reject any equipment that arrives without reference number; however, it may take us longer to process.

Custom requirements for items sent to HyQuest Solutions for warranty or non-warranty repairs: Check with your national customs/tax authorities for details, processes and paperwork regarding tax exempt return of products. Typically, special custom tariff codes are available (such as HS Code = 9802.00) that verify the item is being returned for repair and has no commercial value. Please note that the customs invoice / dispatch documents should also clearly state: "Goods being returned to manufacturer for repair - No Commercial value". It is mandatory to have any returned goods accompanied by a commercial invoice on headed paper. HyQuest Solutions reserves the right to charge the customer for time spent rectifying incorrect customs documents.

Note: Please ensure that your goods are packed carefully and securely. Damage that occurs during transit is not covered by our warranty and may be chargeable.


6.1 TB4 Part List



Note:

The TB4 Series II Rain gauge is ordered with a synthetic ceramic coated brass bucket for 1mm size bucket only or Teflon Impregnated injection moulded non hydroscopic plastic ABS for the 0.1mm, 0.2mm, 0.5mm or 0.01".

Rain gauge Part No.	Rain gauge Description
TB4/0.1/Series II/T	Tipping Bucket Rain gauge, bucket capacity 0.1mm, bucket type Teflon Impregnated injection moulded non hydroscopic plastic ASA UV stabilised
TB4/0.2/Series II/T	Tipping Bucket Rain gauge, bucket capacity 0.2mm, bucket type Teflon Impregnated injection moulded non hydroscopic plastic ASA UV stabilised
TB4/0.01/ Series II/T	Tipping Bucket Rain gauge, bucket capacity 0.01inch, bucket type Teflon Impregnated injection moulded non hydroscopic plastic ASA UV stabilised
TB4/0.5/ Series II/T	Tipping Bucket Rain gauge, bucket capacity 0.5mm, bucket type teflon impregnated ASA plastic UV stabilised
TB4/1.0/M/ Series II	Tipping Bucket Rain gauge, bucket capacity 1.0mm, bucket type synthetic ceramic coated brass

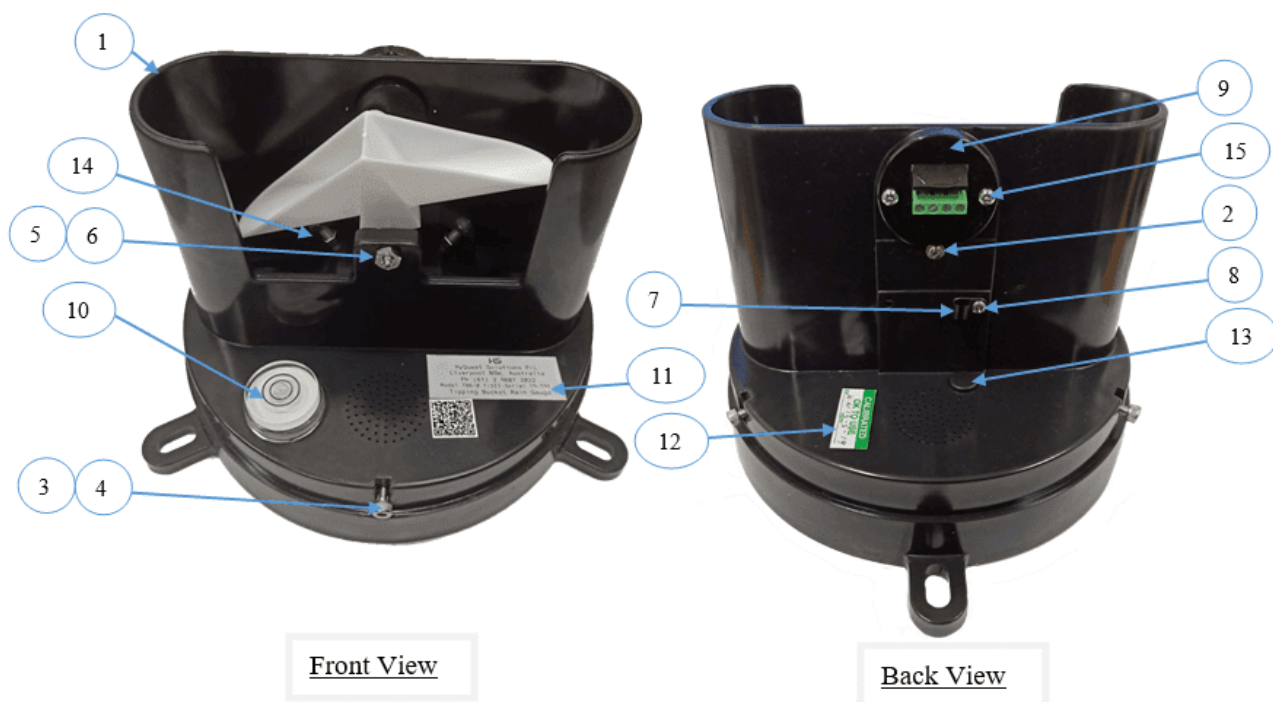

REFERENCE	PART_ID	DESCRIPTION	QTY_PER
1	TB701-01	BASE-INJECTION MOULDED	1
2	TB701-03	BRASS INSERT	2
3	SC008-29	M5x0.8 SS304 HEX NUT	3
4	SC045-21	SOC HD CAPSCREW M5x0.8x12 SS304	3
5	TB301-05	PIVOT SCREW	2


REFERENCE	PART_ID	DESCRIPTION	QTY_PER
6	TB301-06	PIVOT SCREW LOCK NUT	2
7	SC006-12	MINIATURE P CLIP #20-PTC 6.4B	1
8	SC022-114	6GA x 1/4 SELF TAPPING SCREW 304 PAN HD PHILLIPS STAINLESS STEEL	1
9	TB307	MODEL TB3 RAIN GAUGE 24V REED SWITCH ASSEMBLY	0.5
10	SC023-09	BULL'S EYE LEVEL	1
11	SC100-09	SERIAL PLATE	1
12	SC100-06	CALIBRATED LABEL	1
13	SC040-58	SPFM10 10MM FINNED SNAP IN PLUG BLACK	1
14	TB312	ADJUSTING SCREW ASSEMBLY	2
15	SC022-116	6GA x 1/2 SELF TAPPING SCREW 304 PAN HD PHILLIPS STAINLESS STEEL	2

TB4 Series II Bucket Part List

16

Part no: TB304/0.2P/TEF
Descript: Bucket (0.2mm, 0.01")
or
Part no: TB304/0.2P/TEF
Descript: Bucket (0.5mm)

Quantity: 1

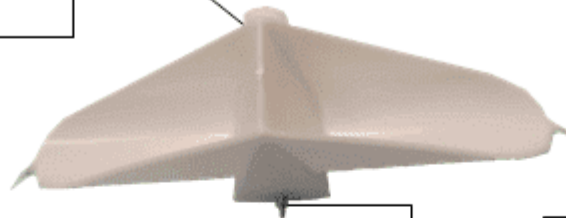

Teflon Impregnated
ASA UV Stabilised
Plastic

17


Part no: TB304-03
Descript: Bucket Axle
Quantity: 1

OR

18

Part no: TB306
Descript: Bucket (1.0mm)

Quantity: 1

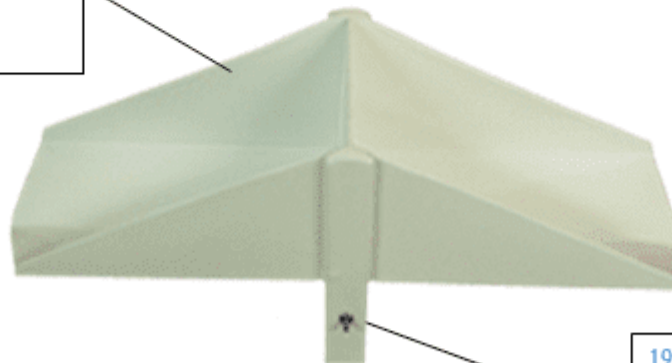


Metal Bucket
1mm only


19

Part no: TB304-03
Descript: Bucket Axle
Quantity: 1


Syphon Part List

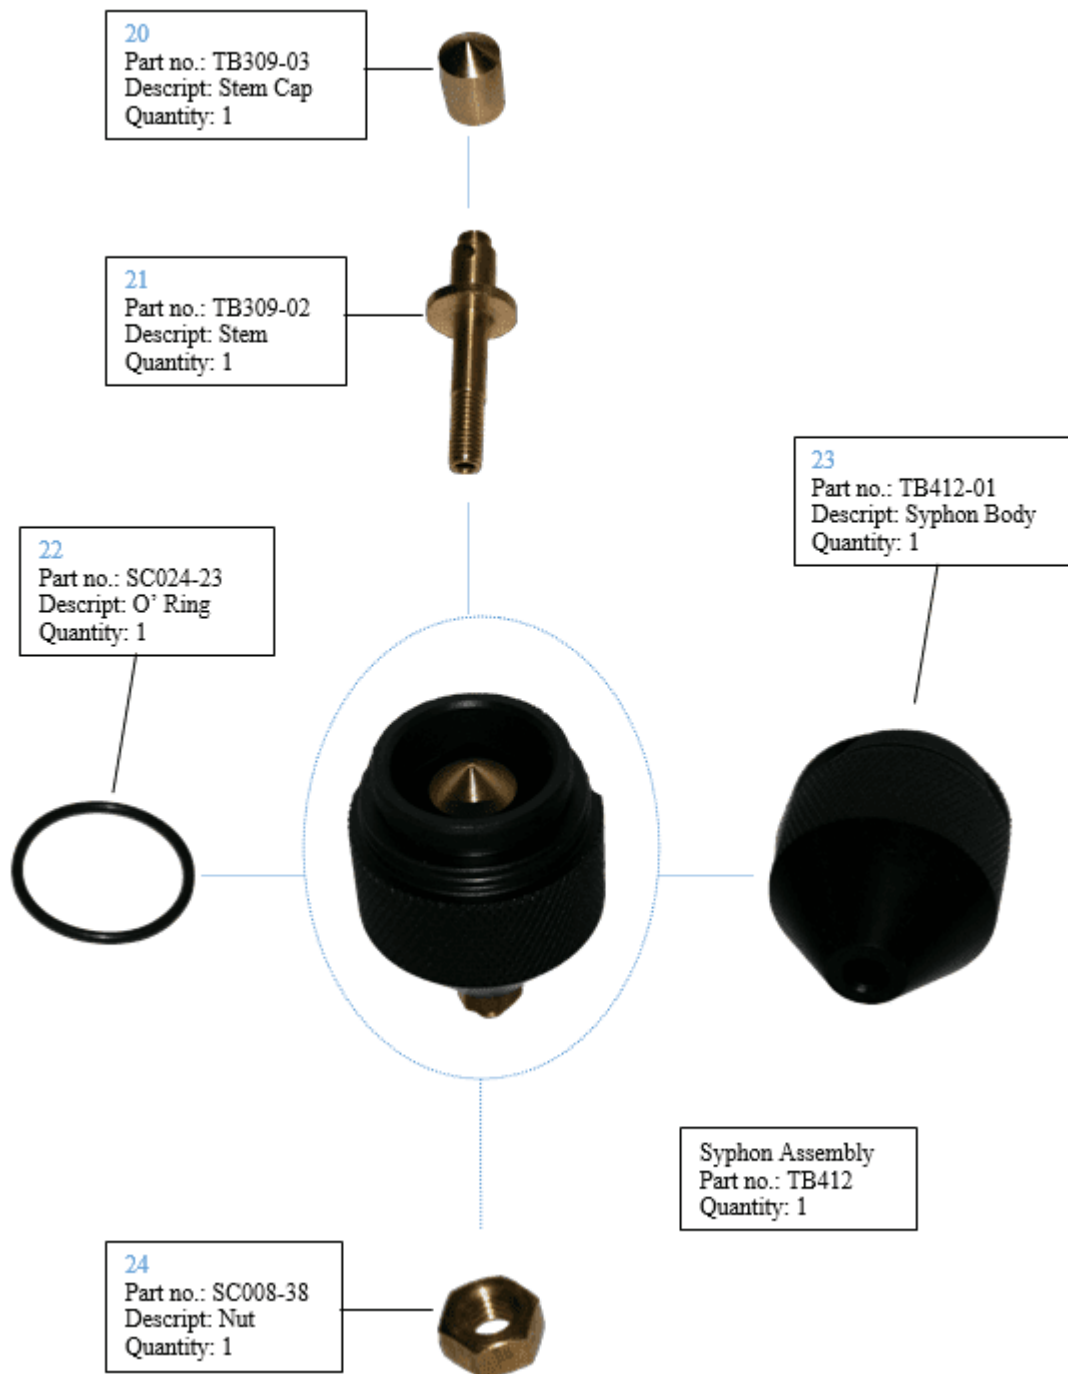

Filter Part List

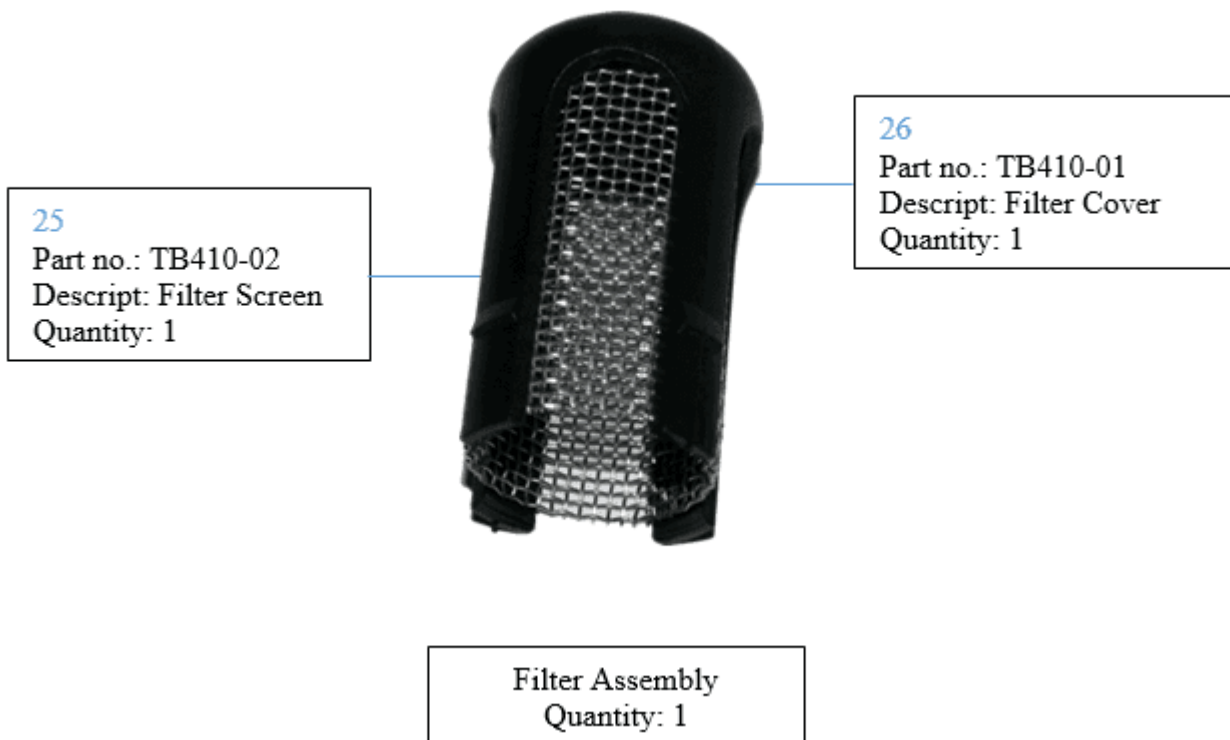

Enclosure Part List

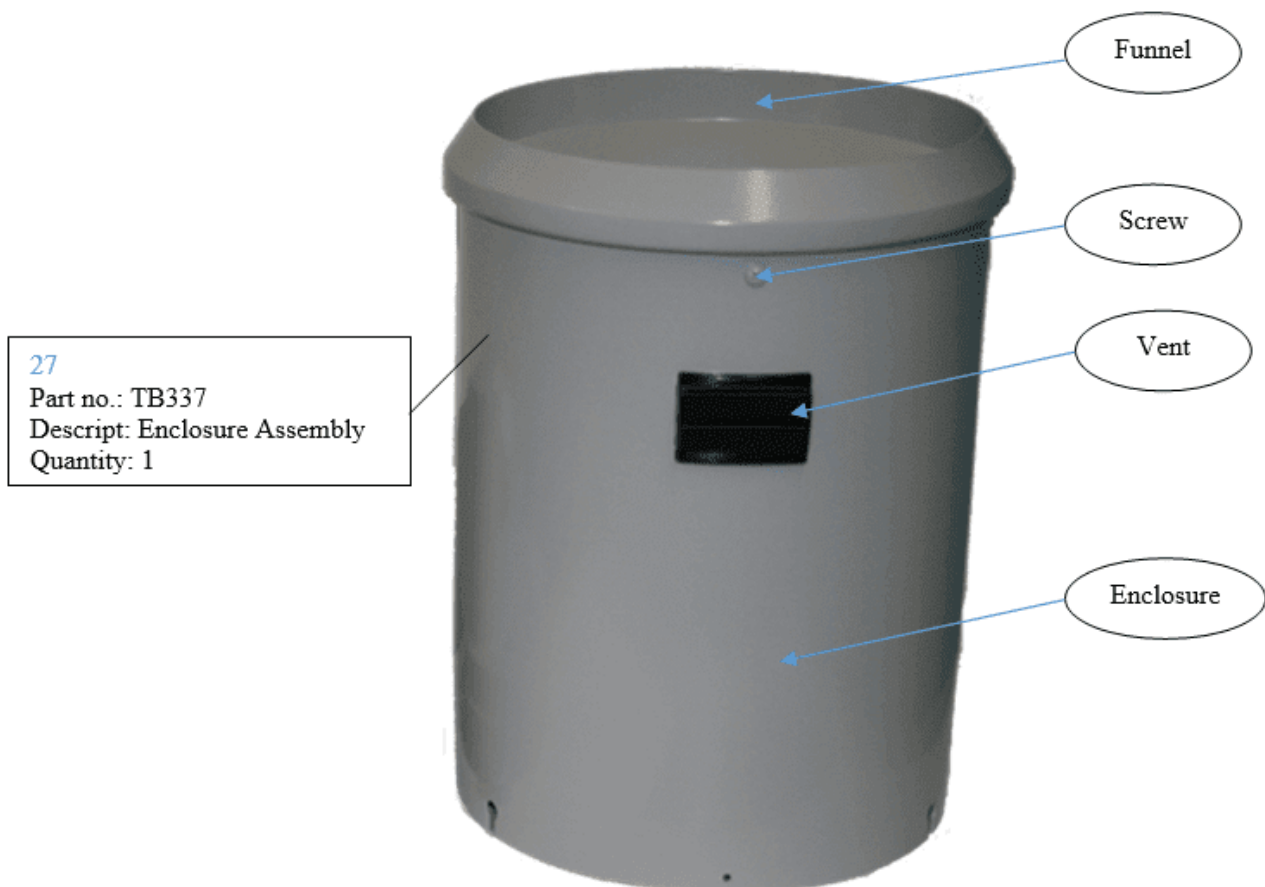

Part no.	Description	Quantity
TB337-01	Funnel	1
TB337-02	Enclosure	1
TB418-06	Vent	1
SC022-72	Screw	3

TB337 breakdown assembly

7 Technical Data

Resolution	0.1 mm	0.2 mm, 0.5 mm, 1.0 mm, 0.01 inch	1.0 mm
Catch Diameter	282.84 mm	200 mm	
Bucket	Teflon-impregnated ASA plastic UV-stabilized or synthetic ceramic-coated brass		Synthetic ceramic-coated brass
Pivot/Bucket Mechanism	Machined, robust stainless steel axle resting on corrosion-free sapphire pivots		
Enclosure and Base	Anodized, powder-coated aluminium		
Accuracy	0 - 250 mm per hour: $\pm 2\%$ 250 - 500 mm per hour: $\pm 3\%$		
Range	0 - 700 mm/h (maximum intensity: 700 mm/h)		
Operating Temperature	4 to 70 °C		
Operating Humidity	0 to 100 %		
Dimensions and Mass	Ø 282.84 mm × H 410 mm 2.7 kg	Ø 200 mm × H 330 mm 2.2 kg	

8 Obligations of the Operator and Disposal

This chapter contains the following subsections:

- [Obligations of the Operator](#) ²³
- [Dismantling / Disposal](#) ²³

8.1 Obligations of the Operator

European Union

In the Single European Market it is the responsibility of the operator to ensure that the following legal regulations are observed and complied with: national implementation of the framework directive (89/391/EEC) and the associated individual directives, in particular 2009/104/EC, on minimum safety and health requirements for the use of work equipment by employees at work.

Worldwide

Regulations: If and where required, operating licences must be obtained by the operator. In addition, national or regional environmental protection requirements must be complied with, regardless of local legal provisions regarding the following topics:

- Occupational safety
- Product disposal

Connections: Local regulations for electrical installation and connections must be observed.

8.2 Dismantling / Disposal

When disposing of the units and their accessories, the applicable local regulations regarding environment, disposal and occupational safety must be observed.

Before dismantling

- Electrical Devices:
 - Switch off the units.
 - Disconnect electrical appliances from the power supply, regardless of whether the appliances are connected to the mains or to another power source.
- Mechanical devices:
 - Fix all loose components. Prevent the device from moving independently or unintentionally.
- Loosen mechanical fastenings: Please note that appliances can be heavy and that loosening the fastenings may cause them to become mechanically unstable.

Disposal

Operators of old appliances must recycle them separately from unsorted municipal waste. This applies in particular to electrical waste and old electronic equipment.

Electrical waste and electronic equipment must not be disposed of as household waste!

Instead, these old appliances must be collected separately and disposed of via the local collection and return systems.

Integrated or provided batteries and accumulators must be separated from the appliances and disposed of at the designated collection point.


EU WEEE Directive

As players in the environmental market, KISTERS AG and HyQuest Solutions are committed to supporting efforts to avoid and recycle waste. Please consider:











Avoidance before recycling!

Recycling before disposal!



This symbol  indicates that the scrapping of the unit must be carried out in accordance with Directive 2012/19/EU. Please observe the local implementation of the directive and any accompanying or supplementary laws and regulations.

Contact Data

Europe	HyQuest Solutions (KISTERS AG)	 +49 2408 9385 0
		 info@hyquestsolutions.eu
Australia	HyQuest Solutions Pty Ltd	 +612 9601 2022
		 sales@hyquestsolutions.com.au
New Zealand	HyQuest Solutions NZ Ltd	 +64 7 857 0810
		 sales@hyquestsolutions.co.nz
Latin America	HyQuest Solutions (KISTERS LATAM)	 +57 350 575 4079
		 sales-latam@hyquestsolutions.com
North America	Hydrological Services America LLC (KISTERS Group)	 +1 561 459 4876
		 sales-hsa@kisters.net

